

# VIRUS SAMPLING KIT

Nucleic acid testing product



Individual package



Flocking head



Safe and reliable



Easy to break

## TUBE CLASSIFICATION

### Regular type (CG-)

Contain virus preservation solution, test within 48 hours to ensure test results  
**(Red cap)**



### Inactivated type (MH-)


Contains virus preservative + virus inactivating agent  
**(Blue cap)**



Usage: For storage and transportation of virus specimens



# SWAB CLASSIFICATION

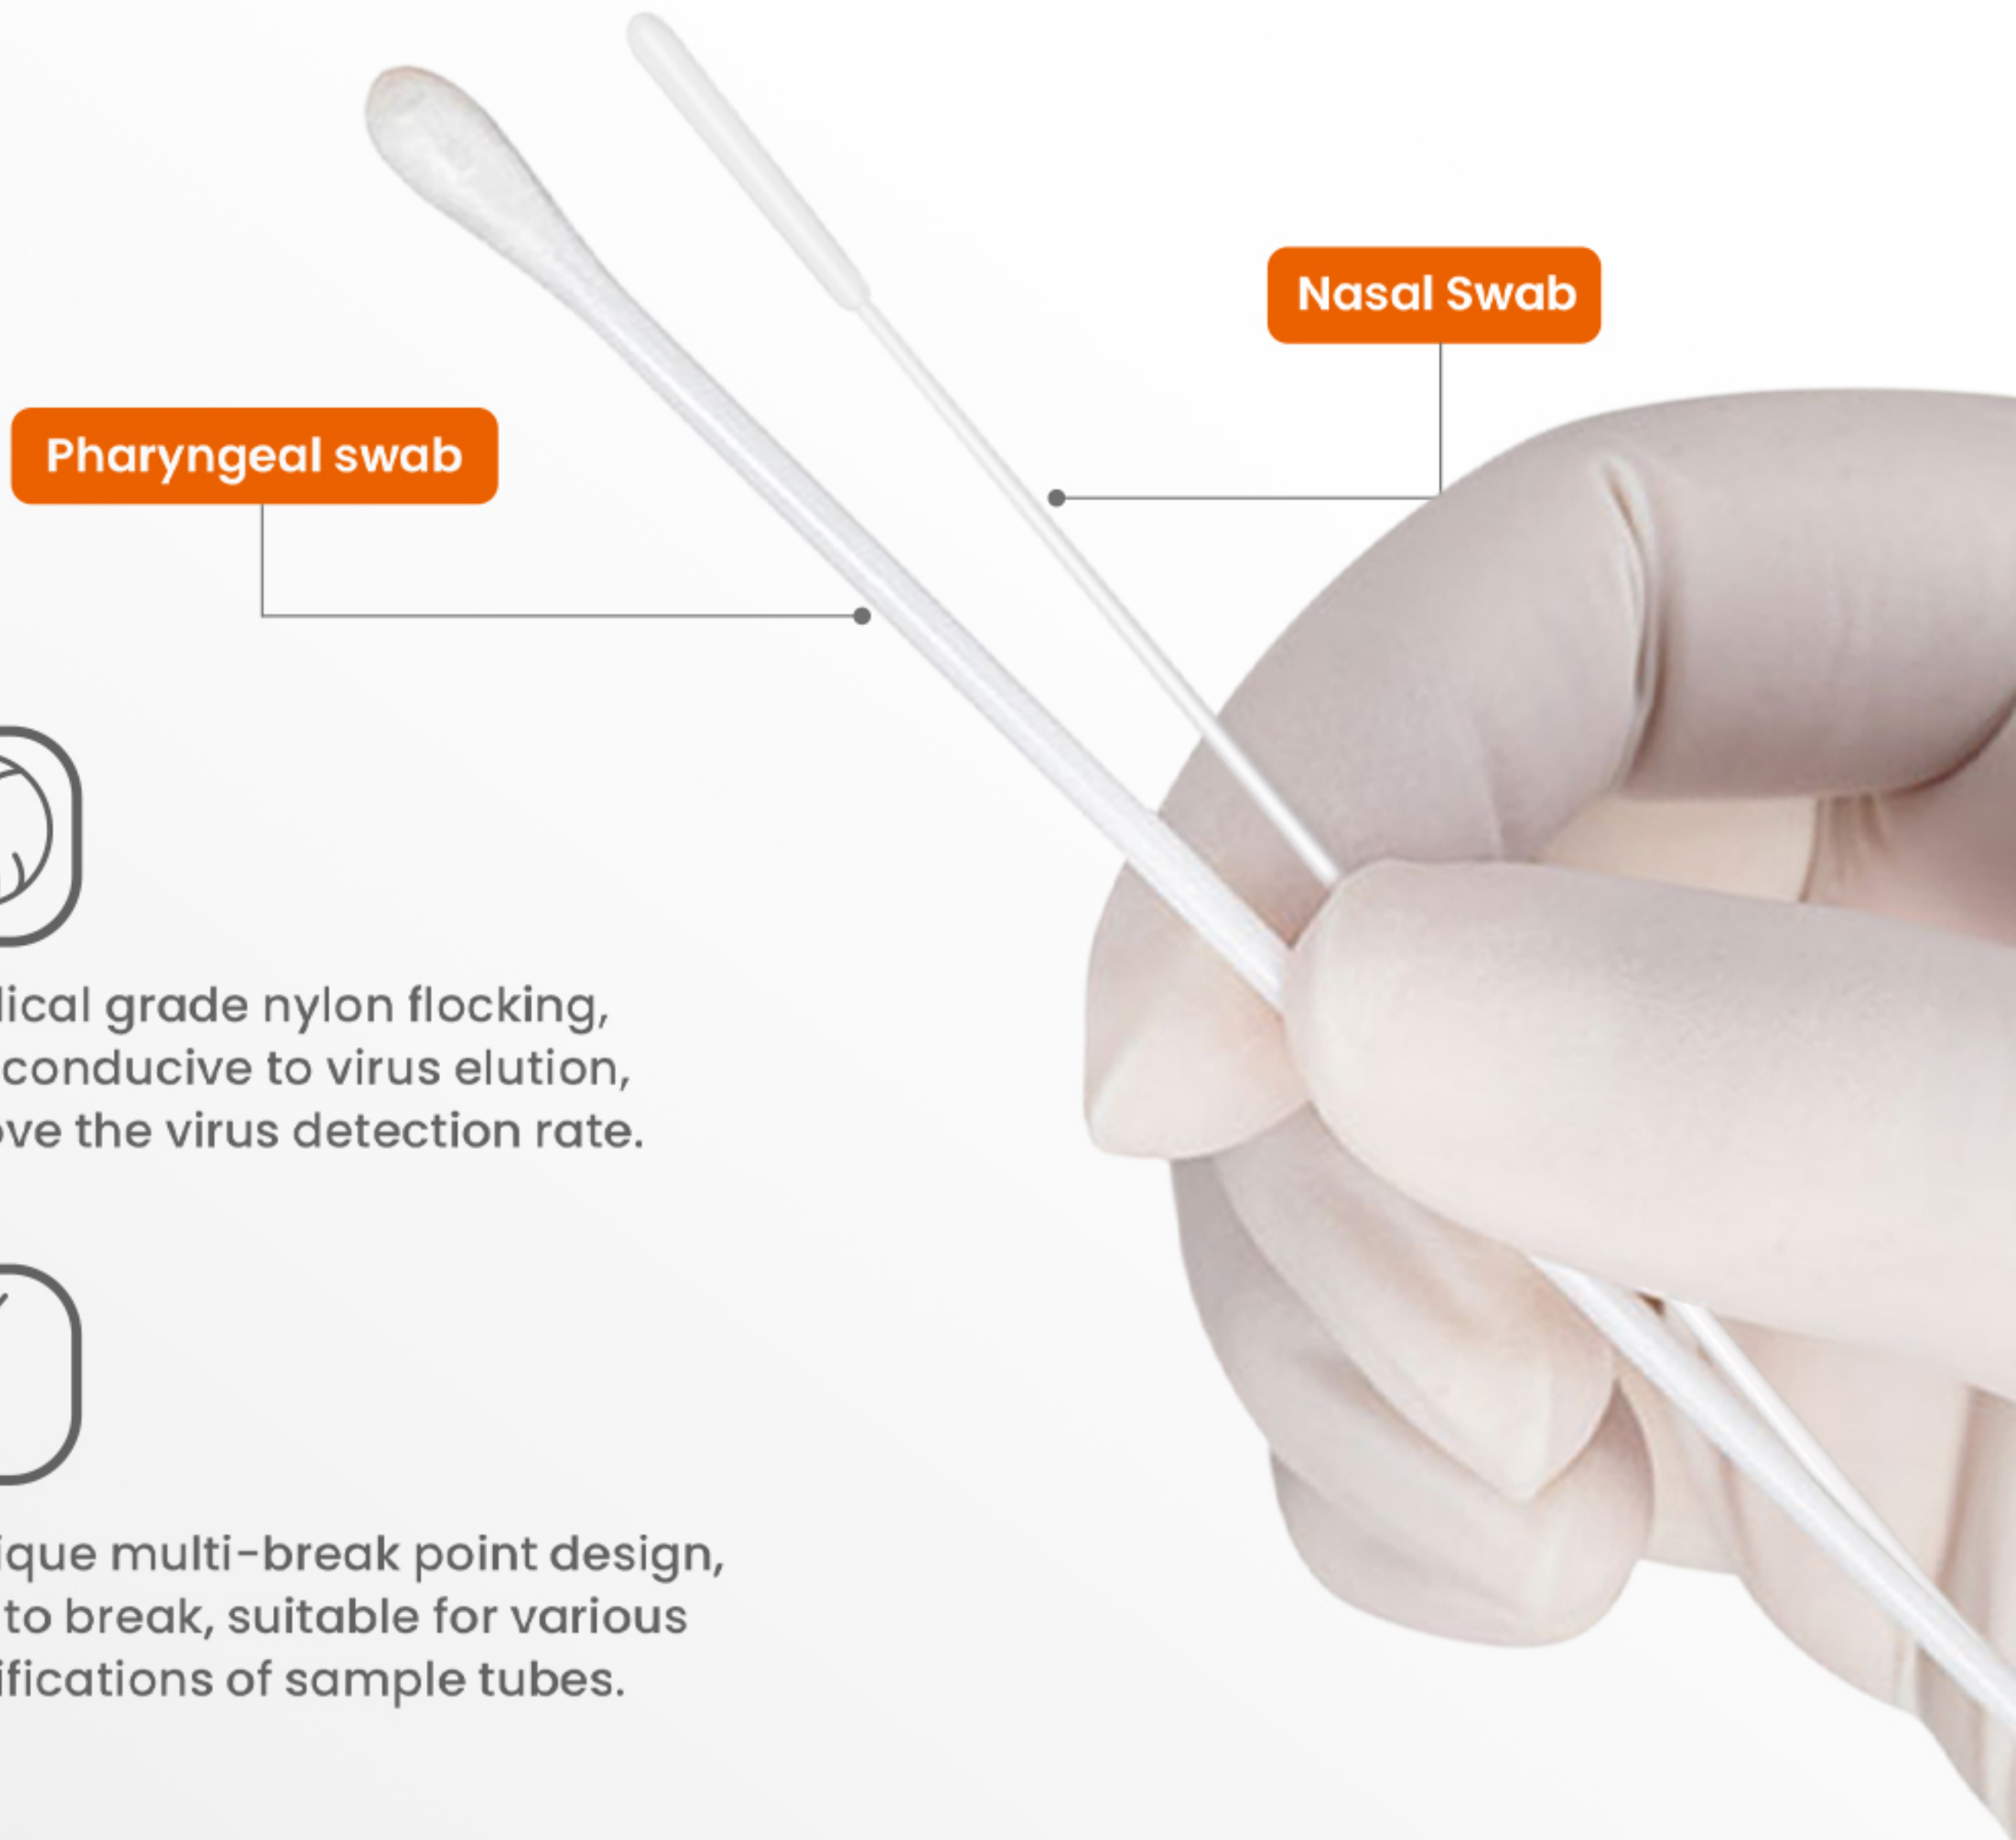

Pharyngeal swab

Nasal Swab



1. Medical grade nylon flocking, more conducive to virus elution, improve the virus detection rate.




2. Unique multi-break point design, easy to break, suitable for various specifications of sample tubes.



## APPLICABLE SCOPE

Collection and delivery of clinical influenza, avian influenza, novel coronavirus, HFMD virus, measles virus and mycoplasma, ureaplasma and chlamydia specimens .

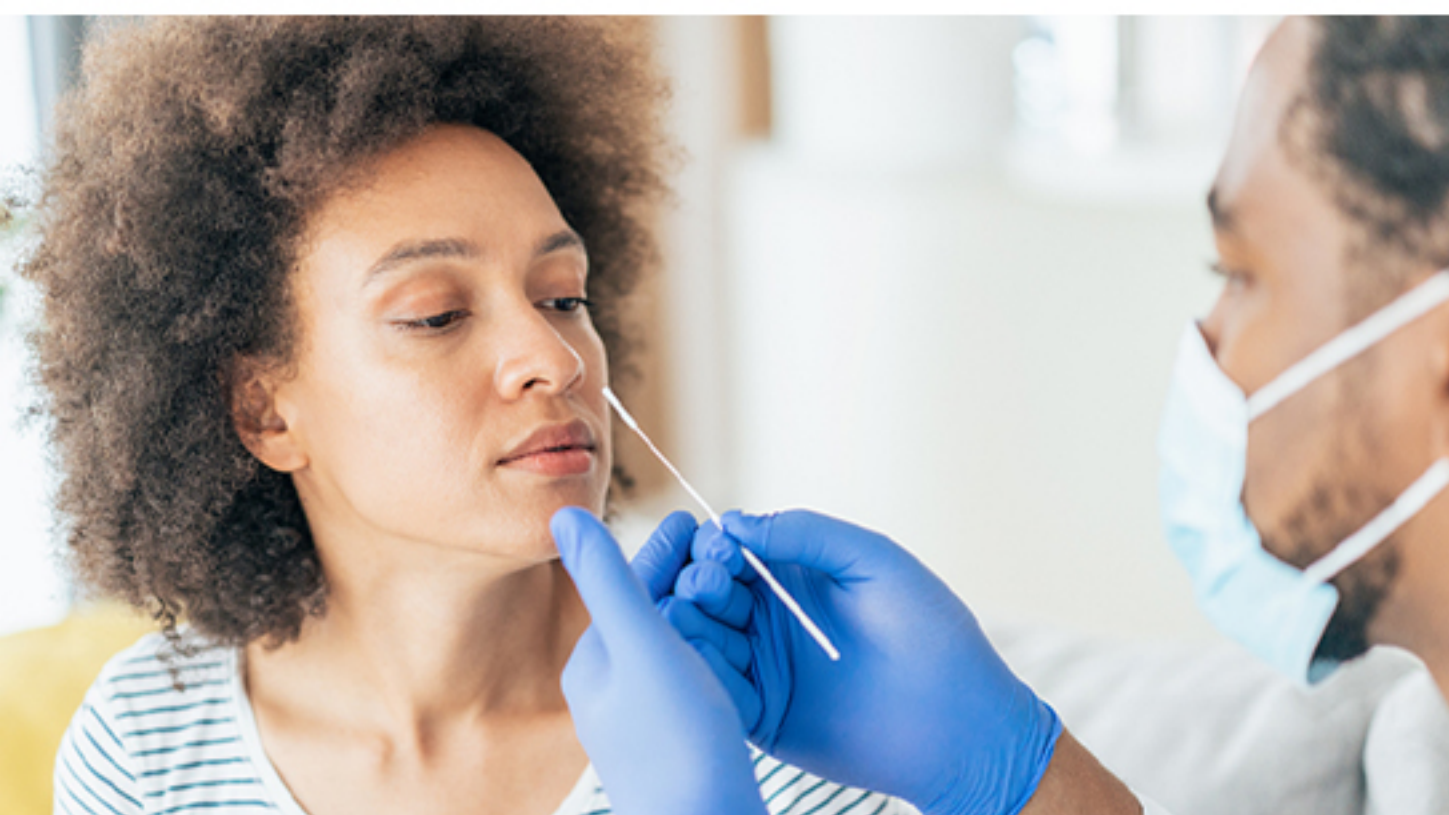

Nasal Sampling



Oral Sampling



# PRODUCT PACKAGING

